




Argon plasma coagulation

with the user-friendly VIO® 3



The benefits of the logical and intuitive VIO 3 interface are now also available with APC 3. As your stepGUIDE, the interface guides you through each menu, suggesting experienced starting settings for APC applications.

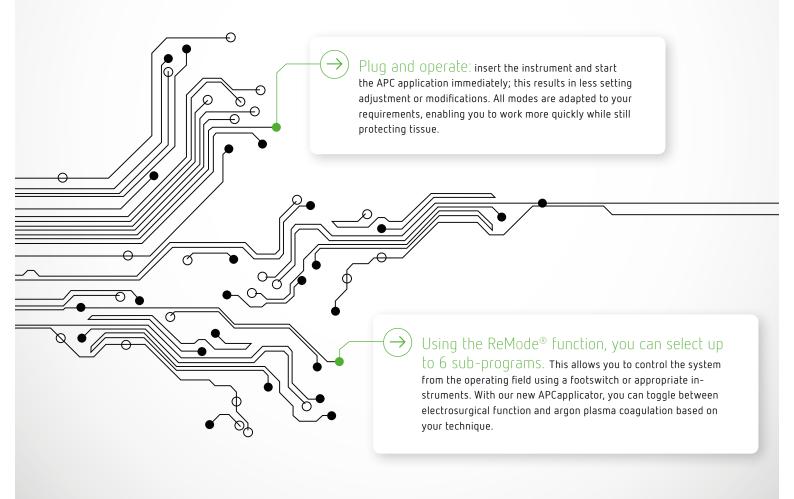



Multi-modality – finely adjustable APC modes



Our APC 3 modes support the full range of APC applications. In addition, the APC 3 facilitates argon-supported cutting, and you can also benefit from the new options offered by our proprietary hybrid technologies — APC combined with our electrosurgical or waterjet technology.

ALL APC MODES ARE INTEGRATED INTO THE VIO® 3:

pulsedAPC® and **forcedAPC** are performed using an even finer, 100-increment effect setting for precisely-adjustable devitalization.

The preciseAPC® mode is used for hemostasis, particularly in the low-energy range and for sensitive structures to facilitate coagulation with minimal penetration.

IT'S NEVER BEEN EASIER:

After selecting a mode, you can adjust the selected mode via the effect setting. It is easy to track the setting configurations and modifications on the large display. Due to precision adjustment, the optimal settings for ablation and coagulation can be refined. The rapid measurement and control technology (logging of 25 million measurements/sec) ensures highly reproducible and homogenous tissue effects.

THE APC SOCKET – YOUR CONNECTION FOR APC FILTERED INSTRUMENTS*


The single use APC instruments can be used for your procedure immediately without time-consuming reprocessing. This is because the filter is already integrated into the connection plug of the FiAPC® probes and of the APCapplicator. "Plug and Operate" thus also stands for immediate availability and utilization of the instruments. The light-weight and easy-to-handle APCapplicator also offers user-friendly activation of all functions with one hand.

APC 3: NOW YOU CAN CONNECT EVEN MORE INSTRUMENTS

Besides the APC socket, an additional multifunctional socket is provided for further instruments. For the first time, this allows you to connect and use up to 6 instruments as required for your procedure.

*FiAPC probe patented: EP 1 515 659 B, US 7,311,707 B, JP 4435680 B, CN 1665451A Design Patents: EP 436274, CN 200630006257.4, US D577,671S, JP 1287552

*APCapplicator with filter Design Patents: EP 2249672, CN ZL201330438131.4, KR 30-2013-0061155 Design patents pending: US 29/475,689

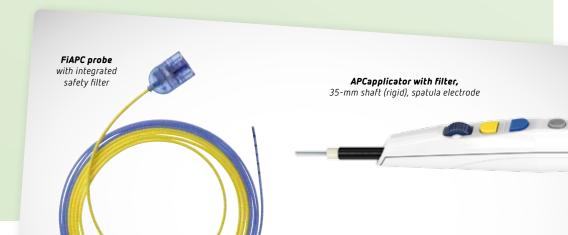

Technical data

Low voltage	Low voltage		Via the VIO 3 electrosurgical unit		
HF		Via the VIO 3 electrosurgical unit			
Potential equalization connection		Yes			
ecific unit data					
Input pressure		(5 ± 2) x 10 ⁵ Pa	5 ± 2 bar	72.5 ± 29 ps	
Max. output pressure		2 x 10 ⁵ ± 2 x 10 ⁴ Pa	2 ± 0.2 bar	29 ± 2.9 psi	
Adjustable gas flow		0.1 – 8 I/min limited by the instrument connected in each case, configurable in 0.1 I/min increments			
Nominal flow tolerance		± 20 % [range: 0.1–8 I/min]			
If you use a compressed	gas cylinder, a warning is activated at	7 x 10⁵ Pa	7 bar	101.5 psi	
Display of remaining quantity		VIO 3 display			
Display of remaining pro	essure	Manometer on the gas cylinder			
The APC 3 switches off	at an input pressure of	< 3 x 10⁵ Pa	< 3 bar	< 43.5 psi	
ions and weight					
Width x height x depth		415 x 100 x 375			
Weight	Weight		5.3 kg		
t conditions for transport	and storage of the unit				
Temperature		-30 °C to +70 °C			
Relative humidity		10 %-90 %			
nt conditions for operating	the unit				
Temperature		+ 10°C - +40 °C			
remperature		15 % – 80 %, non-condensing			
Relative humidity		15 % – 80 %, non-conde	ensing		
`		15 % — 80 %, non-conde	ensing		



Erbe Elektromedizin GmbH Waldhoernlestrasse 17 72072 Tuebingen Germany Phone +49-7071-755-0 Fax +49-7071-755-179 info@erbe-med.com erbe-med.com