

Legend

Important notes


The authors and Erbe Elektromedizin GmbH have taken the greatest possible care while compiling the catalogue with electrosurgical accessories. Nevertheless, it is impossible to exclude the possibility that errors may be contained herein.

The information and recommendations given here may not be construed as constituting any basis for any claims against Erbe Elektromedizin GmbH. Should legal regulations stipulate liability, such liability shall be limited to intentional misconduct or gross negligence.

The data on the use of instruments is based on clinical experience. Medical science is subject to a process of permanent change based on research and clinical experience. Therefore the products are subject to alterations in design and technique. Because of production tolerances dimensions in the catalogue may marginally differ.

We confirm that none of our products contain latex, except the rubber straps, Art. No. 20592-009 and 20592-011.

Further product information

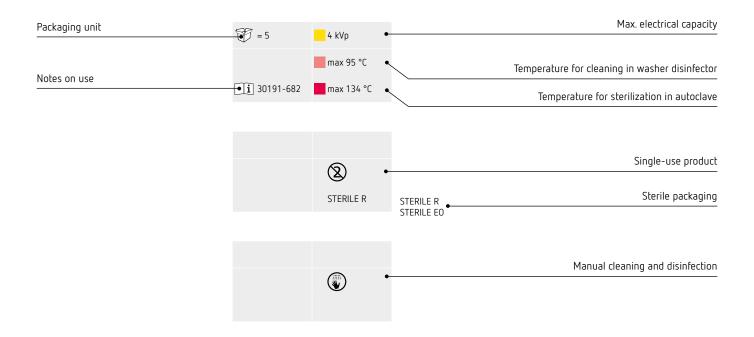

Please read carefully the corresponding notes on use before using any instrument.

Contents

Vessel sealing

Instruments and accessories

- 04 BiClamp
- 12 BiCision
- 13 BiClamp LAP forceps
- 17 BiClamp E LAP forceps
- Accessories for treatment for BiClamp LAP and BiClamp E LAP forceps

Overview

Field of application Shape of instrument BiClamp Laparoscopy BiClamp LAP and BiClamp E LAP Open surgery and laparoscopy BiClision

erbe-med.com

BiClamp







BiClamp





Product type	Length	Shape	Jaws	No.
BiClamp 150 C	150 mm	bent 23°	smooth	20195-221 21195-221
BiClamp 190 C	190 mm	bent 23°	smooth	21195-190
BiClamp 201 T	200 mm	bent 18°	smooth	20195-202 21195-202
BiClamp 210	210 mm	bent 25°	corrugated	20195-200 21195-200
BiClamp 260 C	260 mm	bent 18°	smooth	20195-299 21195-299
BiClamp 271 T	270 mm	bent 18°	smooth	20195-203 21195-203
BiClamp 280	280 mm	bent 25°	smooth	20195-280 21195-280

100 %


BiClamp




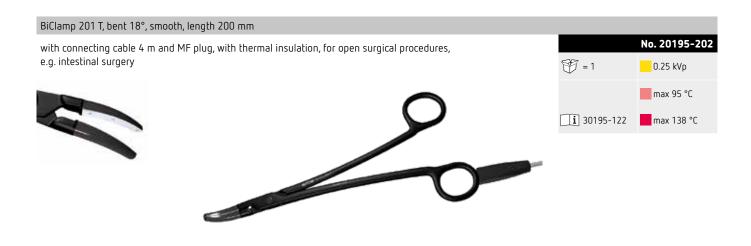


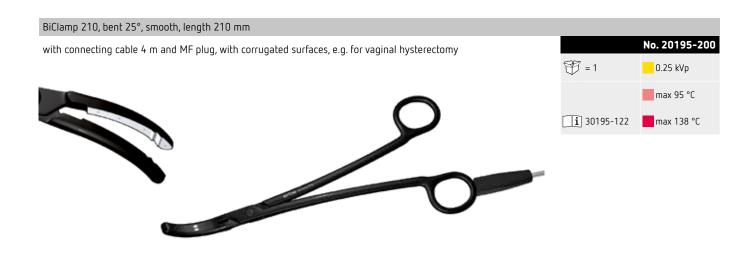

BiClamp

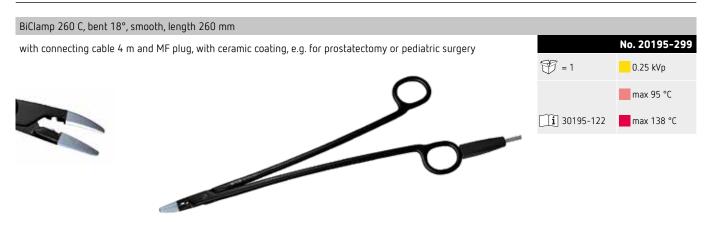


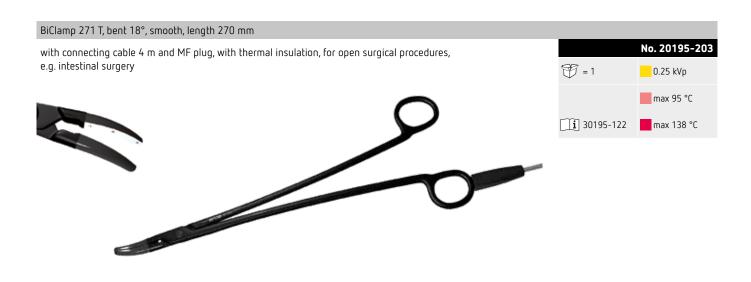


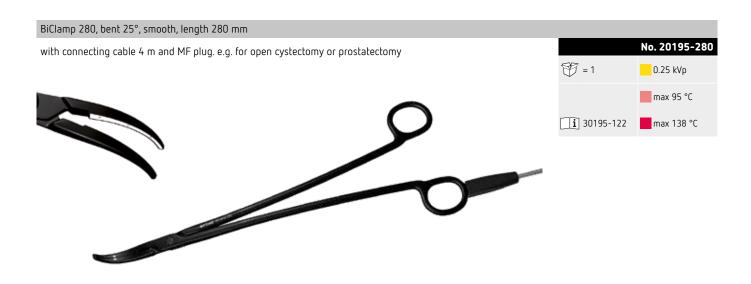


erbe-med.com

BiClamp

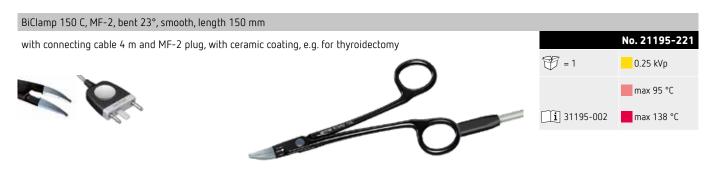


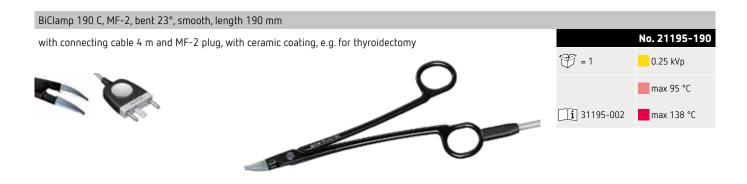


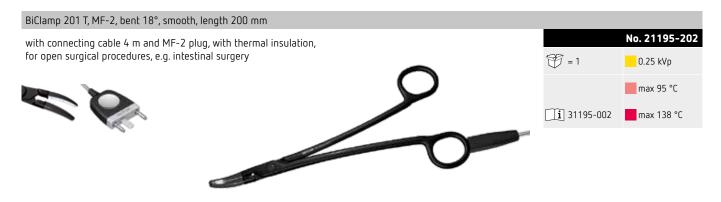




BiClamp

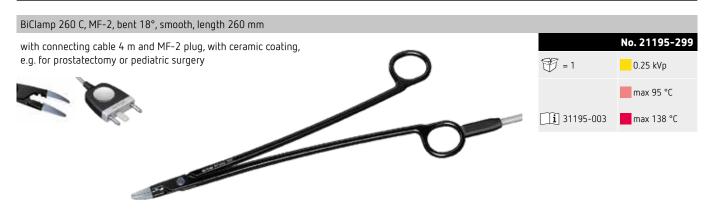

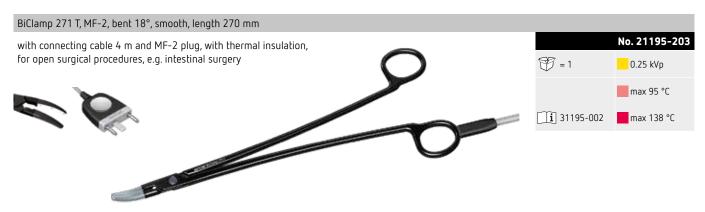


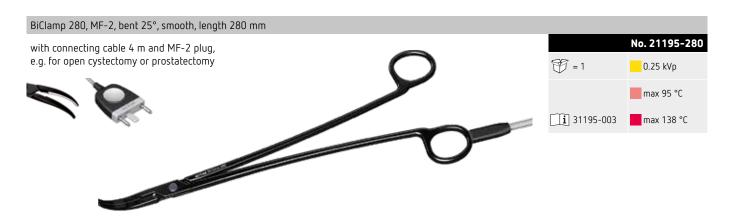



Adapters	Piece	No.
Adapter, MF-socket, MF-2-plug for VIO 300 D	1	20183-100
Adapter, MF-2/MF-U-socket, MF-plug for VIO 3 and VIO 300 D	1	20183-101

erbe-med.com

BiCision

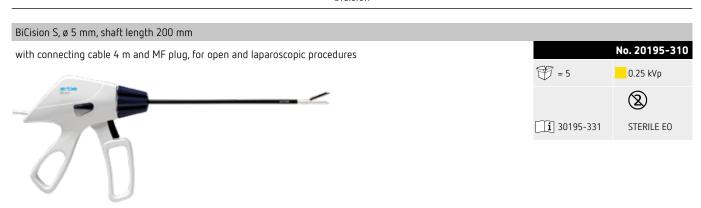

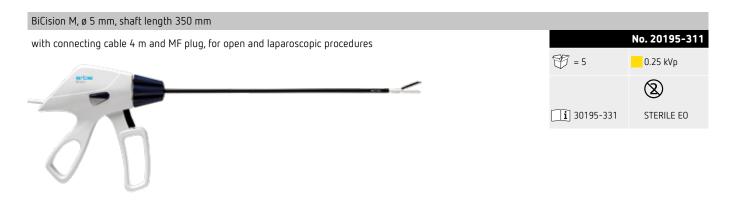

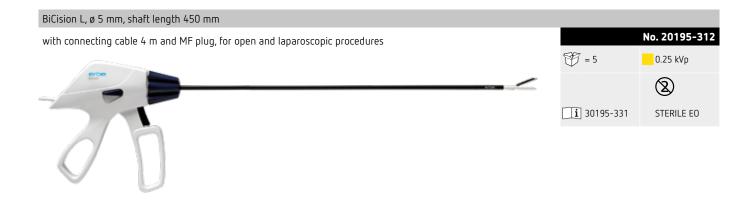

BiClamp LAP forceps










erbe-med.com

BiClamp LAP forceps





BiClamp LAP forceps

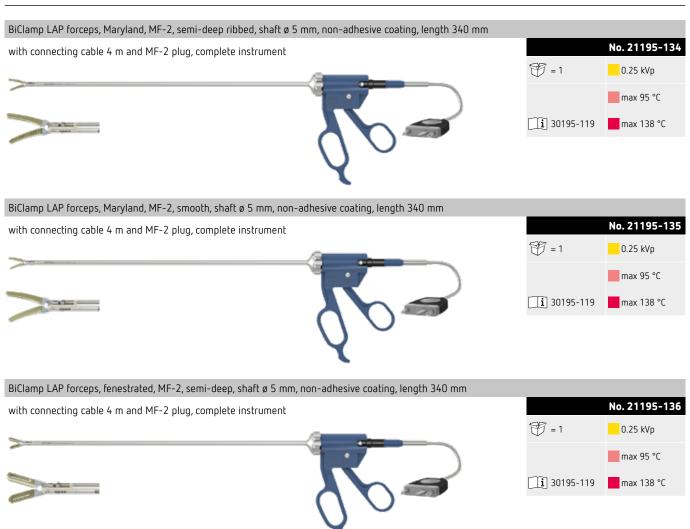





erbe-med.com


BiClamp LAP forceps



Single components		Piece	No.
Insert for BiClamp LAP forceps, Kelly, shaft ø 5 mm, length 340 mm (for 20195-228)	The same surfaces	1	20195-236
Insert for BiClamp LAP forceps, Maryland, semi-deep ribbed, shaft ø 5 mm, length 340 mm (for 20195-134)	- arriva	1	20195-146
Insert for BiClamp LAP forceps, Maryland, smooth, shaft ø 5 mm, length 340 mm (for 20195-135)	The section of	1	20195-147
Insert for BiClamp LAP forceps, fenestrated, semi-deep, shaft ø 5 mm, length 340 mm (for 20195-136)		1	20195-148
Insert for BiClamp LAP forceps, fenestrated, smooth, shaft ø 5 mm, length 340 mm (for 20195-137)		1	20195-149
Insert for BiClamp 110, smooth, shaft ø 5 mm, length 110 mm (for 20195-230)	Table mylan	1	20195-232
Shaft tube for bipolar LAP forceps and BiClamp LAP forceps		1	20195-141
Shaft tube for BiClamp 110, ø 5 mm, length 110 mm (for 20195-230)		1	20195-234
Handle for BiClamp LAP forceps and BiClamp 110, with connecting cable 4 m and MF plug	160	1	20195-145
Handle for BiClamp LAP forceps and BiClamp 110, with connecting cable 4 m and MF-2 plug	160	1	21195-145

Adapters	Piece	No.
Adapter, MF-socket, MF-2-plug for VIO 300 D	1	20183-100
Adapter, MF-2/MF-U-socket, MF-plug for VIO 3 and VIO 300 D	1	20183-101

BiClamp E LAP forceps

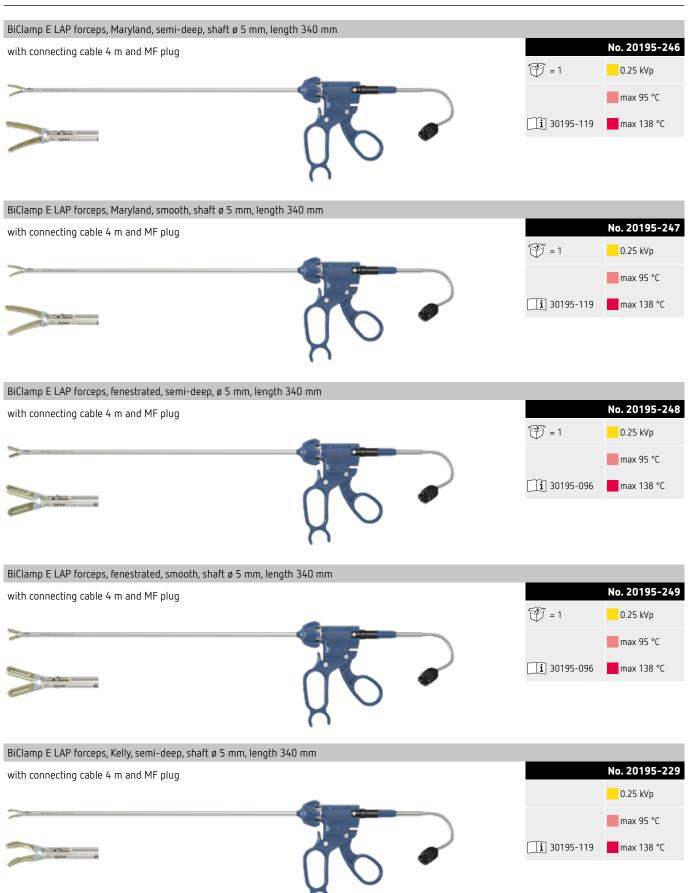

erbe-med.com

BiClamp E LAP forceps











BiClamp E LAP forceps

Single components		Piece	No.
Insert for BiClamp E LAP forceps, Kelly, shaft ø 5 mm, length 340 mm (for 20195-229, 21195-229)	arba arba	1	20195-236
Insert for BiClamp E LAP forceps, Maryland, semi-deep ribbed, shaft ø 5 mm, length 340 mm (for 20195-246, 21195-246)	The section of the se	1	20195-146
Insert for BiClamp E LAP forceps, Maryland, smooth, shaft ø 5 mm, length 340 mm (for 20195-247, 21195-247)	The sections	1	20195-147
Insert for BiClamp E LAP forceps, fenestrated, semi-deep, shaft ø 5 mm, length 340 mm (for 20195-248, 21195-248)	erise	1	20195-148
Insert for BiClamp E LAP forceps, fenestrated, smooth, shaft ø 5 mm, length 340 mm (for 20195-249, 21195-249)	arina	1	20195-149
Shaft tube for BiClamp E LAP forceps, ø 5 mm, length 340 mm		1	20195-241
Handle for BiClamp E LAP forceps, with connecting cable 4 m and MF plug (for 20195-246, 20195-247, 20195-248, 20195-249, 20195-229)	96	1	20195-240
Handle for BiClamp E LAP forceps, with connecting cable 4 m and MF-2 plug (for 21195-246, 21195-247, 21195-248, 21195-249, 21195-229)		1	21195-240

Adapters	Piece	No.
Adapter, MF-socket, MF-2-plug for VIO 300 D		20183-100
Adapter, MF-2/MF-U-socket, MF-plug for VIO 3 and VIO 300 D		20183-101

Accessories for treatment for BiClamp LAP and BiClamp E LAP forceps

Accessories for treatment		Piece	No.
Cleaning brush for suction channel max. ø 3.5 mm, length 650 mm, for manual cleaning and disinfection	4-	1	20191-279
Irrigation tube for shaft tube with Luer Lock connector, length 500 mm, for LAP instruments, for cleaning and disinfection by machine		1	20195-201

erbe-med.com

Important information

We have prepared this document with care. Nonetheless, we cannot completely rule out errors in this document.

The information, recommendations and other data ("Information") contained in this document reflect our state of knowledge and the state of science and technology at the time of preparing the document. The information is of a general nature, non-binding and serves solely for general information purposes and does not represent instructions for use or notes on application.

The information and recommendations contained in this document do not constitute any legal obligations by Erbe Elektromedizin GmbH as well as their associated companies ("Erbe") or any other claims against Erbe. The information does not represent a guarantee or other quality statement, these require the express contractual arrangement with Erbe in individual cases.

Erbe shall not be liable for any type of damage resulting from following information given in this document, regardless of the legal reason for liability.

Every user of an Erbe product is responsible for checking the respective Erbe product for its properties as well as the suitability for the intended type of application or intended purpose in advance. The suitable type of application of the respective Erbe product is given by the user manual and the notes on use for the corresponding Erbe product. The user is obliged to check whether the existing user manual and the notes on use correspond with the status for the specific Erbe product. The devices may only be used according to the user manual and the notes on use.

The information on setting values, application sites, duration of application and the use of the respective Erbe product is based on the clinical experience of physicians independent from Erbe. They represent guidelines which need to be checked by the user for their suitability for the actual planned application. Depending on the circumstances of an actual application case, it may be necessary to deviate from the information provided. The user has to check this on his/her own responsibility in each case when using an Erbe product. We wish to point out that science and technology is constantly subject to new developments arising from research and clinical experience. For this reason it may be necessary for the user to deviate from the information provided in this document.

This document contains information about Erbe products which may possibly not be approved in a specific country. The user of the respective Erbe product is obliged to inform him/herself whether the Erbe product he/she is using is legally approved in his/her country and/or if legal requirements or restrictions for use possibly exist and to which extent.

This document is not intended for users in the USA.

Erbe Elektromedizin GmbH Waldhoernlestrasse 17 72072 Tuebingen Germany

Phone +49 7071 755-0 Fax +49 7071 755-179 info@erbe-med.com erbe-med.com